

Optical Sensors and Their Applications in Medical Fields

Algassim Mohamed Ahmed Abd Albagi¹, Dr. Amin Babiker A/Nabi Mustafa²

^{1,2}Department of telecommunication, Faculty of Engineering, Al Neelain University, Khartoum, Sudan, 2014

Abstract: *Optical techniques developed for sensing purposes proved to be essential in many application fields, ranging from aerospace, industry, process control, to security, and also medicine. The capabilities of these sensors are generally enhanced when a bulk-optical configuration is replaced by optical fibre technology. In the past few years, research programmes and also the market for fibre sensors have assumed a relevant role. This is undoubtedly due to the growing interest in optoelectronics, but also to the very satisfactory performance and reliability that optical fibre sensors are now able to provide. This paper focuses on the advantages that optical fibre sensors offer to the biomedical field.*

Keywords: Optical fibers, optical sensors, pharmaceuticals, total internal reflection

1. Introduction

Fiber optics, though used meticulously in the modern world, is a quite simple and old technology. The principle of light guidance by refraction phenomenon, was first established by Colladon and Babinet in Paris in the early 1840s, as a base for fiber optics[1]. Fiber optics is mainly used for transmitting radiation from one component to another with help of fibers[2]. Optical fibers are fine strands of glass or plastic, single or bunch of which is used for transmission of radiation from one compartment to another to several hundreds of feet, not only for observation purpose, but also for illumination of objects. The essential feature for transmission of light in an optical fiber which occurs by total internal reflection is that the transmitting fiber must be coated with the material that has refractive index smaller (Cladding material) than that of fiber material (Core). The emission of ultra violet, visible or infrared radiations by the fiber depends on the choice of construction material[3].

The transmission of light by total internal reflection along the fiber allows only certain modes for propagation which depend on the diameter of the fiber and the wavelength of the light used. Two types of fibers are offered for a given incident wavelength namely, monomode and multimode. Monomode fibers have a narrow glass core of uniform refractive index profile and transmit only a single mode for light of a specific wavelength range and linearly polarized state. Monomode fibers produce a Gaussian spatial intensity distribution at their distal end, whereas multimode fibers have a greater core diameter and can transmit many a hundreds of light modes having either a uniform or parabolically profiled cross sectional refractive index. It is much easier to commence high intensities into multimodal fibers because of their larger core size and higher numerical aperture, than their monomodal equivalents or counterparts. They do however, have disadvantages related to modal noise. Any thermal or mechanical annoyance to the fiber affects each transmitted mode in a diverse way. As a result, although the total light intensity at the fiber exit remains constant, the far field radiation pattern formed by intervention of these modes changes with time[4].

Unlike glass or plastic, the varied materials of construction are silica, fluorides, phosphates and chalcogenide. The construction of model optical fiber initiates with the development of large diameter preform of desired refractive index, pulling from which produces a long thin optical fiber. The preform is commonly made by three chemical vapour deposition methods: Inside vapour deposition, outside vapour deposition, and vapour axial deposition[5]. Extensively used phosphate glass can be advantageous over silica glass for optical fibers with a high concentration of doping rare earth ions for the transmission of radiations. A mixture of fluoride glass and phosphate glass is fluorophosphate glass, which is not associated with the disadvantage of modal noise[6,7].

2. Sensor Systems and Sensor Types

The simplest partition of optical sensors is into so called intrinsic devices, where the interaction occurs actually within an element of the optical fiber itself and extrinsic devices where the optical fiber is used to couple light, usually to and from the region where the light beam is influenced by the substance which is being measured[8].

2.1 Luminescent Optical Fiber Sensors

The use of luminescent phenomena, directed chiefly on fluorescence for optical sensing, has been observed with a range of diverse fiber hosts. Evidently, those rare earths, which have been doped most usually into silica based fibers, or alternatively into fluoride glass or more unusual fiber materials, can evenly be applied to the generation of simple fluorescence as to the creation of laser action. However, unlike the plastic host that has disadvantage of quenching laser action, there are ample varieties of other fluorescent materials which can be used for sensing purpose, where their primary focus is only on the fluorescence. A key distinction between silica and plastic fiber is the extreme elasticity of the latter, which allows it to bent to a greater extent with a smaller radius than silica fiber[9].

2.2 Evanescent Wave Fluorescent Sensor

A negative or non-guiding fiber is a permeable fiber in which the power loss depends on the length of the fiber and can be optimized for fluorescence collection efficiency into the positive or guiding fiber attached to the output end of the negative fiber. This is in contrast to the positive fibre for which the collection efficiency is independent of fibre length and depends only on the difference in refractive index between core and cladding material of the fiber. The sensor described is based on a fiber having two different fibres, one guiding and other non-guiding. The combination of a guiding fibre and a non-guiding fibre can detect fluorescence emitted from molecules attached to the surface of the negative fibre as shown in fig. 1[10,11].

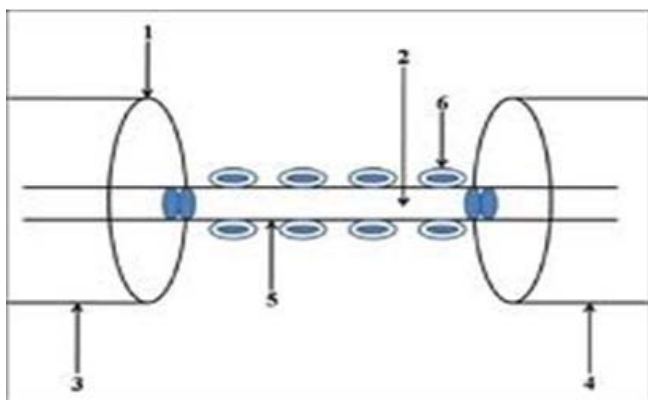


Figure 1: Fiber based evanescent fluorescent sensor The combination of a guiding fibre (1) and a non-guiding fibre (2) can detect fluorescence emitted from molecules attached to the surface of the core of the negative fibre with the help of sensing element (5) ...

2.3 Thin film sensors

The presence of immobilizing enzyme layers of glucose oxidase on chalcogenide fibers lead to the novel concept of IR fiber optical chemical sensors to analyse glucose in complex aqueous matrices. The sensing design is based on following the catalyzed reaction of glucose to gluconic acid and hydrogen peroxide. Monitoring the concentration of reaction products in the surrounding aqueous solution by evanescent wave spectroscopy believe an enzyme layer thinner than the penetration depth of the irradiation but with maximum reactivity of the catalytically active surface to offer a fast sensor response. Hence a careful treatment of the fiber surface with 3 aminopropyltriethoxysilane (APTS)/glutaraldehyde before immobilizing the enzyme is apparent [12,13]. A newer approach by Taga *et al.* improves the enzyme density on the fiber surface was developed by immobilizing glucose oxidase via bacterial S-layer protein[14].

2.4 Fluorescent plastic optical fiber sensors:

Fibers in this category are characteristically doped with organic dyes which are used extensively in the printing industry and for display purposes. They are frequently used for decorative purposes, but clad (dressed) and coated fibers with a fluorescent core are often used in sensing and measurement as a result of their ability to capture light,

which excites them over their whole length. The kind of fluorescent sensors are used to measure ambient light[15], monitor faults in circuits and switches[16], humidity measurement[17], environment sensing and detection of gaseous pollutants[18].

3. Applications

Fibre optic sensors have numerous applications in diverse branches of science and engineering, as is evident from a vast range of properties which has been sensed optically, ranging from light intensity, vibration, temperature, pressure, calibration of accelerometers, strain, liquid level, pH, chemical analysis, concentration, density, refractive index of liquids etc[19,20]. Refractometer are frequently used for the study of molecular structure and identification of organic compounds[21,22]. The overall general applications of optical fibers are described in Table 1.

Table 1: General Applications of Optical Fibers

Application of optical fibers in various industries

Communications
Pharmaceuticals
Spectroscopy
Biological and biomedical sciences
Petrochemicals
Food and beverage industry
Plastic industry
Study of soil samples
Understanding the basic chemical reactions
Energy and military services

3.1 Glucose Sensor

Earlier times, ultra violet radiation and immobilized probes were used for sensing purpose[23,24], but nowadays a fiber based pH meter has been developed in which the cladding material is replaced with polyaniline polymer, a polymer with broad sensitivity to pH[25]. Since only a single broad band is to be measured, the system adapts itself to an IR laser diode system which offers a potential for miniaturization and greater portability. Brown *et al.* modified the sensor by using glucose oxidase immobilised on the polyaniline polymer surface (an enzyme which converts glucose to glucuronic add, resulting in a pH change) to predict glucose concentration [26].

3.2 Laminate Cure Analysis

Monitoring reactions in hostile environment becomes much easy with these probes having smaller dimensions and enough durability. Fiber optic probes can be introduced into an autoclave (via the usually standard thermocouple calibration port) and thus can continuously monitor the progress of reactions (e.g. degradation) as a function of the operating conditions. Druy *et al.* utilized this approach to monitor ongoing processes in industries, notably to monitor

heal rates of polymer laminates at higher temperature and pressures [27,28].

3.3. Protein Analysis

Fiber optic sensors are useful for protein analysis since high quality spectra can be obtained from low concentrations of analyte in a variety of environments without any interference. Globular proteins usually exhibit regions of secondary structure including alpha helices, P-sheets, turns and non-ordered regions. Each of these conformational entities contributes to the IR spectrum in the amide I contour region. In addition to the study of protein in its dried state, FTIR coupled with fiber optic probes has been particularly useful for the study of soluble proteins, whose structures had not previously been elucidated using X-ray diffraction or NMR spectroscopy[29,30].

3.4 Dosage Form Analysis

Reported the application of an optical fiber probe for quality control in the pharmaceutical industry[31]. The system was used to quantitatively determine the content of a number of pharmaceutical solid dosage forms containing ibuprofen, and powders containing benzydamine an analogue of cetrimide. A team from Burroughs-Wellcome have taken this one step ahead and have performed identification tests on tablets through the plastic wall of the blister packaging[32] to distinguish between film coated and uncoated tablets and between active and placebo forms. The technique satisfied the requirements of a confirmation of identity test prior to use in a clinical trial[33].

3.5 Fiber optical scanning in TLC for drug identification

Proposed an organized toxicological analysis procedure using high-performance thin layer chromatography in combination with fibre optical scanning densitometry for recognition of drugs in biological samples. The technique allowed parallel recording of chromatograms by identifying the drugs and comparing their ultra violet spectra with the data obtained from library as a reference spectra[34].

3.6 Determination of DNA oligomers

Demonstrated the binding of DNA oligonucleotides to immobilized DNA targets using a fiber optic fluorescence sensor. 13 mer oligonucleotides were attached to the core of a multimode fiber and the complementary sequence was identified by using a fluorescent double stranded specific DNA ligand. The evanescent field was used to differentiate between bound and unbound species. The template DNA oligomer was immobilized either by direct coupling to the activated sensor surface or using the avidin biotin bridge to detect the single base mismatches in the target sequence [35].

3.7 Effluent Monitoring

Reported the environmental hazard associated with the use of chlorinated hydrocarbons by pharmaceutical manufacturers[37,38]. Chlorohydrocarbons have their strongest absorption bands and therefore polycrystalline

silver halide fibers are of value as light guides. For quantitative measurements, the 10 cm fiber collectors were coupled to the FTIR and samples were monitored. Further study revealed the comparative analysis of tetrachlorethylene and waste water samples showing a good concord with standard gas chromatographic techniques[39].

3.8 Other Applications

Fiber optic probe is not only used for the determination of water by near infrared reflectance spectroscopy[40] but also for determination of penicillamine in pharmaceuticals and human plasma by capillary electrophoresis with in column fiber optics light emitting diode induced fluorescence detection[41]. Fiber lasers are also used for the military applications, biological and biomedical applications and highly sensitive airborne trace gas detection [42,43].

Applications that are made possible by the use of filtered fiber optic Raman probes include such things as measuring high levels of organic solvent contaminants in soils and aquifers, chemical process monitoring of petrochemicals and distillation products, monitoring polymer cure reactions in situ and many others[44–45].

In spectroscopy, in order to analyse the composition of substance that cannot be placed into the spectrometer itself can be measured by optical bundles by transmitting the light from a spectrometer to a substance. A spectrometer analyzes substances by bouncing light off of and through them. By using fibers, a spectrometer can be used to study objects that are too large to fit inside, or gases, or reactions which occur in pressure vessels [46].

4. Future Perspectives

With such an ongoing demand of optical fibers in the science world, novel techniques like such fiber optic probes in Raman and Attenuated Total Reflectance can be used for communications, military and defense, sensing and biomedical imaging. These probes can also help in the authentication of the drug product, and thus preventing the drug counterfeit.

5. Conclusions

An optical fiber made up of a core carries the light pulses which are not only used for sensing but also for the illumination purpose. Fiber optic probes undergo total internal reflection and aid in possible future biomedical applications to carry out the simultaneous collection and analysis of samples for drug safety evaluation. It also helps in the sensing of biomolecules, identification of drug molecules, effluent monitoring and overall pharmaceutical quality control of the product. Probes aid in the development of kinetics profile and are associated with short sample times, allowing the identification and measurement more accurate and reliable.

References

- [1] Bates RJ. New York: McGraw Hill publishers; 2001. Optical Switching and Networking Handbook; p. 10.
- [2] Optical waveguides. Photon plumbing for the chemistry lab: Fiber optics wave guides and evanescent waves as tools for chemical analysis. *Anal Chem.* 1982; 54:1071A–80.
- [3] Skoog DA, Holler FJ, Crouch SR. Belmont, CA: Brooks/Cole Cengage learning; 2007. Instrumental Analysis. India ed; p. 233.
- [4] Macfadyen AJ, Jennings BR. Fibre optic systems for dynamic light scattering –a review. *Optics Laser Technol.* 1990;22:175–87.
- [5] Gowar J. 2nd ed. Hempstead UK: Prentice Hall; 1993. Optical communication systems; p. 209.
- [6] Karabulut M. Mechanical and structural properties of phosphate glasses. *J Non-Cryst Solids.* 2001;288:8.
- [7] Kurkjian C. Mechanical properties of phosphate glasses. *J Non-Cryst Solids.* 2000;207:263–64.
- [8] Zhang ZY, Grattan KT. Survey of US patent activity in optical fiber sensors. European Workshop on Optical Fibre Sensors. SPIE. 1998;3483:218–22.
- [9] Grattan KT, Sun T. Fiber optic sensor technology: An overview. *Sens Actuators.* 2000;82:40–61.
- [10] Glass TR, Lackie S, Hirschfeld T. Effect of numerical aperture on signal level in cylindrical waveguide evanescent fluoro-sensors. *Appl Opt.* 1987;26:2181–7.
- [11] Ahmad M, Chang K, King TA, Hench LL. A compact fiber based fluorescence sensor. *Sens Actuators A.* 2005;119:84–9.
- [12] Taga K, Kellner R. 8th Fourier transform spectroscopy, Conf. SPIE Proc. 1992;1575:238–40.
- [13] Kellner R, Taga K. Optical science and engineering. SPIE Proc. 1991;1510:232.
- [14] Taga K, Kellner R, Kainz U, Sleytr UB. In situ attenuated total reflectance FT-IR analysis of an enzyme-modified mid-infrared fiber surface using crystalline bacterial surface proteins. *Anal Chem.* 1994;66:35–9.
- [15] Grattan KT, Meggitt BT. London: Kluwer Academic Publishing; 1998-2000. Optical Fiber Sensor Technology; pp. 1–5.
- [16] Augousti AT, Mason J, Grattan KT. A simple fiber optic level sensor using fluorescent fiber. *Rev Sci Instrum.* 1990;61:3854.
- [17] Muto S, Fukasawa A, Kamimura M, Shinmura F, Ito H. Fiber humidity sensor using fluorescent dye-doped plastics. *Jpn J Appl Phys.* 1989;28:1065.
- [18] Sawada H, Tanaka A, Wakatsuki N. Plastic optical fiber doped with organic fluorescent materials. *Fujitsu Sci Techno J.* 1989;25:163.
- [19] Binu S. Calibration of accelerometers by using an extrinsic fiber optic probe. *Microw Opt Technol Lett.* 2007;49:2700.
- [20] Culshaw B. Optical systems and sensors for measurement and control. *J Phys E.* 1983;16:978.
- [21] Karrer E, Orr RS. A Photoelectric Refractometer. *J Opt Soc Am.* 1946;36:42. [PubMed]
- [22] Ross IN, Mbanu A. Optical monitoring of glucose concentration. *Opt Laser Technol.* 1985;17:31.
- [23] Jones, Porter MD. Optical pH sensor based on the chemical modification of a porous polymer film. *Anal Chem.* 1988;60:404–6.
- [24] Zhang S, Tanaka S, Wickramsighe YA, Rolfe P. Fiber-optical sensor based on fluorescence indicator for monitoring physiological pH values. *Med Biol Eng Comput.* 1995;33:152–6.
- [25] Ge ZF. Fiber optic near and mid infrared spectroscopy and clinical applications. *Diss Abstr Int.* 1995;55:3855.
- [26] Brown, Chen Near and mid infrared chemical and biological sensors. *Proc SPIE Int Sot Opt Eng.* 1995;2506:243–50.
- [27] Druy, Glatkowski, Stevenson WA. Proc. ADPA/AIAA/ASME/SPIE. UK: IOP Publishers; 1992. Embedded optical fiber sensors for monitoring cure cycles of composites.
- [28] Druy, Glatkowski, Stevenson WA. Mid IR tapered chalcogenide fiber optic attenuated total reflectance (ATR) sensors for monitoring epoxy resin chemistry. *SPIE Int Soc Opt Eng.* 1993;2089:114–20.
- [29] Mantele W. Reaction induced infra-red spectroscopy for the study of protein function and reaction mechanisms. *TIBS.* 1993;18:197–202. [PubMed]
- [30] Mantele W. Reaction induced infra-red spectroscopy for the study of protein function and reaction mechanisms. *TIBS.* 1993;18:197–202. [PubMed]
- [31] Dreassi E, Ceramelli G, Corti P, Massacesi M, Perruccio PL. Quantitative Fourier transform near infra red spectroscopy in the quality control of sold pharmaceutical formulations. *Analyst.* 1995;120:2361–5.
- [32] MacDonald BF, Gemperline PJ, Boyer NR. A near infrared reflectance analysis method for the non invasive identification of film coated and non film coated, blister packed tablets. *Chim Acta.* 1995;310:43–51.
- [33] Blanco M, Coello J, Iturriaga H, MasPOCH S, Russo E. Control analysis of a pharmaceutical preparation by near infrared Dempster reflectance spectroscopy. A comparative study of a spinning module and a fiber optic probe. *Anal Chim Acta.* 1994;298:183–91.
- [34] Ahrens B, Blankenhorn D, Spangenberg B. Advanced fibre optical scanning in thin layer chromatography for drug identification. *J Chromatogr B.* 2002;772:11–8. [PubMed]
- [35] Kleinjung F, Bier, Axe, Warsinke, Frieder W, Scheller Fibre-optic genosensor for specific determination of femtomolar DNA oligomers. *Anal Chim Acta.* 1997;350:51–8.
- [36] Rajan, Chand S, Gupta BD. Surface plasmon resonance based fiber optic sensor for the detection of pesticide. *Sens Actuators B.* 2007;123:661–6.
- [37] Krska R, Rosenberg E, Taga K, Kellner R, Messica A, Katzir A. Polymer Coated silver halide infrared fiber as sensing devices for chlorinated hydrocarbons in water. *Appl Phys Lett.* 1992;61:1778–80.
- [38] Krska R, Taga K, Kellner R. Simultaneous in situ trace analysis of several chlorinated hydrocarbons in water with an IR fiber optical system. *J Mol Structure.* 1993;294:1–4.
- [39] Krska R, Taga K, Kellner R. New IR fiber optic chemical sensor for in situ measurements of chlorinated hydrocarbons in water. *App Spect.* 1993;47:1484–7.

- [40] Blanco M, Coello J, Iturriaga H, MasPOCH S, Rovira E. Determination of water in ferrous lactate by near infrared reflectance spectroscopy with a fiber optics probe. *J Pharm Biomed Anal.* 1997;16:255–62. [PubMed]
- [41] Yang X, Yuan H, Wang C, Su X, Hu L, Xiao D. Determination of penicillamine in pharmaceuticals and human plasma by capillary electrophoresis within column fiber optics light emitting diode induced fluorescence detection. *J Pharm Biomed Anal.* 2007;45:362–6. [PubMed]
- [42] Richter D, Fried A, Wert BP, Walega JG, Kittel FK. Development of a tunable mid IR difference frequency laser source for highly sensitive airborne trace gas detection. *Appl Phys B.* 2002;75:281–8. [PubMed]
- [43] Greenwald J, Rosen S, Anderson RR. Comparative histological studies of the tunable dye (at 577 nm) dye laser and argon laser: The specific vascular effects of the dye laser. *J Invest Dermatol.* 1981;77:305–10. [PubMed]
- [44] Lyon RE, Chike KE, Angel SM. In situ cure monitoring of epoxy resins using fiber-optic probe. *J Appl Polym Sci.* 1994;53:1805.
- [45] Garrison AA, Moore CF, Roberts MJ, Hall PD. Distillation process control using fourier transform raman spectroscopy. *Process Control Qual.* 1992;3:57–63.
- [46] Mosheky Z, Melling PJ, Thomson MA. In situ real time monitoring of a fermentation reaction using a fiber optic FT-IR probe. *Spectroscopy.* 2001;16:15. Available from: <http://www.remspec.com/pdfs/SP5619.pdf>.