

Valuation of Radiation Dose in Lumbosacral Examination

Yousif Mohamed Y. Abdallah^{1,2}, Maryem Milad Hemair³, Amel S. Algaddal⁴

¹ College of Medical Radiological Science, Sudan University of Science and Technology, Khartoum, Sudan

² College of Applied Medical Science, Almajmah University, Riyadh, KSA

³ Faculty of Medical Technology, Alzawya University, Alzawya, Libya

⁴ Sebha Infertility Center, Sebha, Libya

Abstract: The biological damage produce by radiation is closely related to the amount of energy absorbed in the case of x-rays. Measurement of produced ionizing is provided a useful assessment of the total energy absorbed. This study was performed in Khartoum teaching hospital in period of January to June 2014. This study performed to assess the effective dose (ED) received in lumbosacral radiographic examination and to analyze effective dose distributions among radiological departments under study. The study was performed in Khartoum teaching hospital, covering two x-ray units and a sample of 50 patients. The following parameters were recorded age, weight, height, body mass index (BMI) derived from weight (kg) and (height (m)) and exposure factors. The dose was measured for lumbosacral x-rays examination. For effective dose calculation, the entrance surface dose (ESD) values were estimated from the x-ray tube output parameters for Lumbosacral Spine AP and lateral examinations. The ED values were then calculated from the obtained ESD values using IAEA calculation methods. Effective doses were then calculated from energy imparted using ED conversion factors proposed by IAEA. The results of ED values calculated showed that patient exposure were within the normal range of exposure. The mean ED values calculated were 2.49 ± 0.03 and 5.60 ± 0.22 for Lumbosacral Spine AP and lateral examinations, respectively. Further studies are recommended with more number of patients and using more two modalities for comparison.

Keywords: radiation dose, radiation protection, lumbosacral imaging

1. Introduction

Worldwide the number and range of x-ray facilities and x-ray equipment is increasing rapidly, in recent years, diagnostic radiology has witnessed and enormous rise in the number of types of interventional radiology [1-2]. In addition Computed tomography scanning has become widely available with some center now possessing machines capable of helical scanning which have potentially high patient through put. All these factors have contributed to a large increase in frequency of x-ray examination. In Europe, diagnostic radiology represents largest man. Made contribution to population doses [3-4]. This observation is also applies to both developing countries alike. Patient dosimetry is now regarded as an integral part of quality assurance program. National Radiological Protection Board guidance levels or reference doses have been recommended by various organization as a means of patient dose reduction. International commission on radiation units measurements defined absorbed dose as the amount of energy deposited in a medium per unit mass [5-8]. When the medium is air and photon energies with in the diagnostic range, air kerma and absorbed dose are almost equal. However, this does not apply when other media such as tissue or water are considered. It is common practice to attach dosimeters to the skin during a patient dose survey. These dosimeters may measure either entrance surface dose (ESD) in a given media or entrance surface air kerma (ESAK) if entrance surface dose is specified in air then [9-10]. Digital fluoroscopy, digital subtraction angiography, digital spot imaging and conventional fluoroscopy system present particular problems for patient. Examination performed on these type of

equipment are almost in variably under taken under some degree of automated control of technique factors. as a result, the technique factor stand to change continually during the examination. In addition the area irradiated by the primary beam also changes during the examination. In this dose area product or air kerma area product correlate reasonably well with radiation risk, as the number of interactions with in the patient is proportional to both dose or air kerma and field size [11-14].

2. Methods and Materials

This study involved 50 patients undergoing lumbar spine radiographic examinations in different radiology departments at Khartoum teaching Hospital in period of June to December 2014. The radiographic equipment used was Toshiba and shimadzu imaging system. The target angle for the X-ray tube was 12° , and the measured ripple for tube potential was in the region of 1%. Total filtration for the X-ray system measured as 2.7 mm of aluminum equivalent. ESDs in this study were calculated using the following equation:

$$ESD = OPx \left(\frac{kV}{80} \right)^2 x mAsx \left(\frac{100}{FSD} \right)^2 BSF$$

Where:

(OP) is the output in mGy/ (mA) of the X-ray tube at 80 kV at a focus distance of 1 m normalized to 10 mA s, (kV) the tube potential, (mA) the product of the tube current (mA) and the exposure time(s), (FSD) the focus-to-skin distance (in cm). (BSF) the backscatter factor, the normalization at 80 kV and 10 mAs was used as the potentials across the X-ray tube

and the tube current are highly stabilized at this point. The results were tabulated in the Tables (Mean \pm Standard Deviation (SD).

3. The Results

For the group of patients where age distribution was measured, 24 % of patients were within the 15-25 years age range, 12 % of patients were within the 26-35 years age range, 16 % of patients were within the 36-45 years age range, 28 % of patients were within the 46-55 years age range, 20 % of patients were within the 56-65 years age range. The key parameters for this group are shown in Fig. 1.

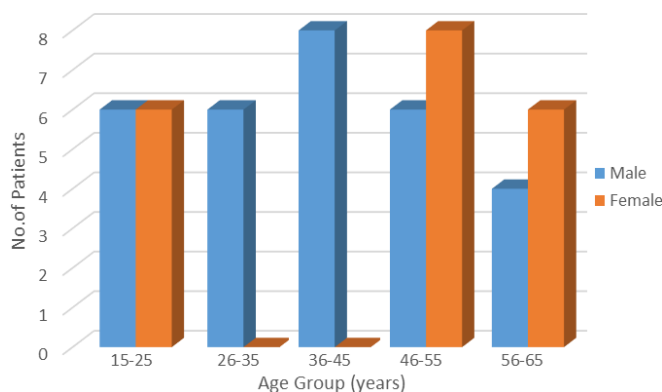


Figure 1: Age Distribution in Sample

For the group of patients where Body Mass Index (BMI) was measured, 24 % of patients were within the $1.9 + .44$ (male), $2.07 + 0.78$ (female) BMI ratio range, 12 % of patients were within the $2.08 + 0.50$ (male) BMI ratio range, 16 % of patients were within the $2.6 + 0.28$ (male) BMI ratio range, 28 % of patients were within the $2.6 + 0.28$ (male) and $2.8 + 0.59$ (female) BMI ratio range, 20 % of patients were within the $3.2 + 0.21$ (male) and $3.14 + 1.44$ (female) BMI ratio range. The key parameters for this group are shown in Fig. 2.

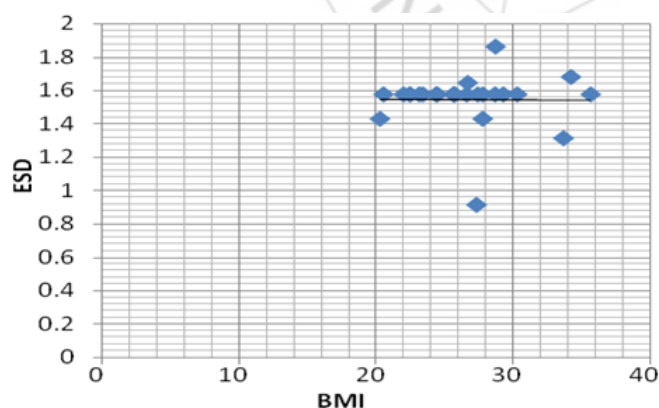


Figure 2: Relationship between entrance skin dose ESD (mGy) and body mass index BMI (Kg/m²) of patients undergoing LS X-ray

For the group of patients where x-rays exposure factors (kVp and mAs) was measured, 24 % of patients were within the $82.0 + 5.9$ (kVp), $52.6 + 17.3$ (mAs) exposure factors ratio range, 12 % of patients were within the $82.1 + 34.6$ (kVp) and $59.6 + 16.2$ (mAs) exposure factors ratio range, 16 % of patients were within the $85.6 + 8.8$ (kVp) and $58.7 + 21.8$ (mAs) exposure factors ratio range, 28 % of patients were

within the $85.4 + 8.07$ (kVp) and $79.8 + 23.8$ (mAs) exposure factors ratio range, 20 % of patients were within the $87.1 + 6.8$ (kVp) and $75.7 + 24.1$ (mAs) exposure factors ratio range. The correlation between the entrance skin dose ESD (mGy) and tube potential kVp in (kVp) to patients undergoing LS X-ray this group were shown in fig. 3.

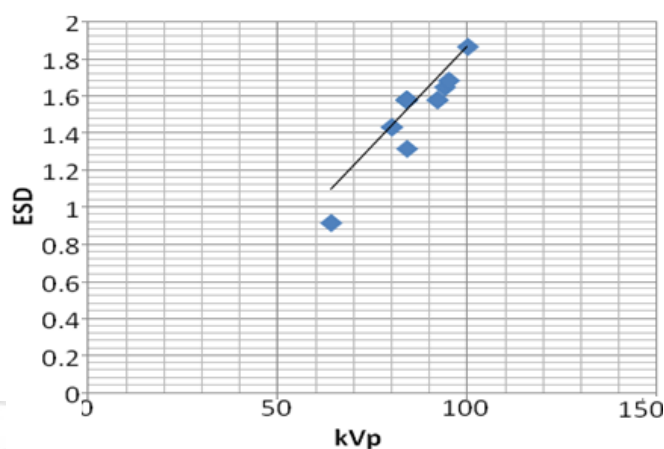


Figure 3: Relationship between entrance skin dose ESD (mGy) and tube potential (kVp).

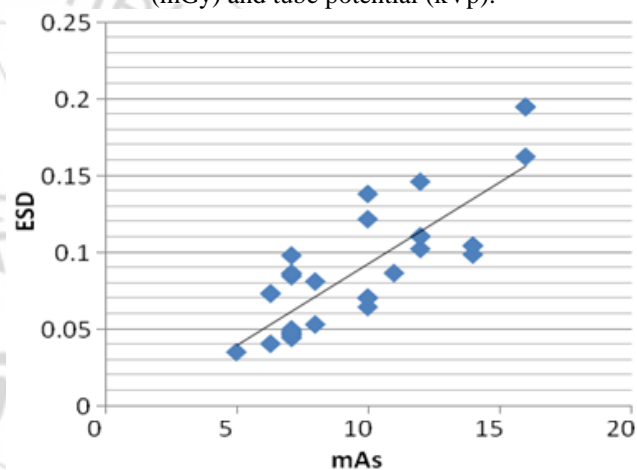


Figure 4: Relationship between entrance skin dose ESD (mGy) and tube current (mAs).

The measured dose was $2.49 + 0.03$ mGy and 5.60 ± 0.22 for anteroposterior and lateral projection respectively.

4. Conclusion

In this study it was found that doses for L/S for the entire examination were higher AP/LS and LA/LS respectively. Unlike other trails, the dose in L/S radiography was higher in conventional radiography compared to other techniques. Recently digital and computed radiography are becoming more popular due to the important advantage of digital imaging is cost and access. The image quality met the criteria of the departments for all investigation. Further studies are recommended with more number of patients and using more two modalities for comparison and dose optimization during CR imaging must be considered.

References

- [1] Al-Shawi, A. K. and Fern, E. D, 2003, The tent drape for the c-arm image intensifier. Injury, July: 12.

- [2] Mesbahi A. and Rouhani A., 2008, Study on the radiation dose of the orthopaedic surgeon and staff from a min C-arm fluoroscopy unit. J radiation protection dosimetry; 10.1093:1-4.
- [3] Bahari S, Morris S, Broe D, Taylor C, Lenehan B, Mcelwain J., 2006, Radiation exposure of the hands and thyroid gland during percutaneous wiring of wrist and hand procedures. Acta Orthop. Belg. 72, 194-198.
- [4] Bushberg, J. T., Seibert, J. A, Leidholdt, E. M. and Boone, J. M 2003. The Essential Physics of Medical Imaging. 2nd ed. Lippincott William and Wilkins, Philadelphia. USA.
- [5] Dowd, B. S. and Tilson, E. R. 1999. Practical Radiation Protection and Applied Radiobiology. 2nd ed. Pennsylvania: Sunders Company.
- [6] Edward J.C, Ernest Fawzy, Jakub Kaczynski, Phillip Hassman, Simon H. Palmer, 2010, A comparative study of radiation dose and screening time between mini C-arm and standard fluoroscopy in elective foot and ankle surgery. Foot and ankle surgery.
- [7] Compagnone G, M Casadio Baleni, L Pagan, F L Calzolaio, L Barozzi, and C ergamini, 2006, Comparison of radiation doses to patients undergoing standard radiographic examinations with conventional screen-film radiography, computed radiography and direct digital radiography. British Journal of Radiology 79, 899-904.
- [8] Osman H, Suleiman A., Suliman I., Sam A., 1996, Radiation Dose Measurements in routine X ray Examinations. Arab Journal of Nuclear Science- Egypt .
- [9] Hart D., Hillier M.C., Wall B.F., 2010, Dose to patients from medical x-ray /examinations in the UK-1995 review, NRPB-R289, London: HMSO. Henner Anja, Radiographer students learning dose management of the patients, Proceedings of Third European IRPA Congress 2010 June 14–18,
- [10] Helsin ki, Finland,(2010). Henshaw PS, Hawkins JW. Incidence of leukemia in physicians. J Natl Cancer Inst 1944; 4:339–346.
- [11] Herrmann KA, Bonél H, Stabler A, Kulinna C, Glaser C, Holzkecht N, 2002, Chest imaging with flat-panel detector at low and standard doses: comparison with storage phosphor technology in normal patients. Eur Radiol;2:385–90. I. I.
- [12] Suliman, N, Abbas, and F.I. Habbani, 2007, Entrance surface dose to patients undergoing selected x-ray diagnostic examinations in Sudan. Radiat. Prot . Dosim.123 (2), 209–214.
- [13] Jones, D. G. and Stoddart, J. 1998. Radiation use in the orthopaedic theater: a prospective audit. Australian and New Zealand Journal of Surgery. Nov. 68(11): 782-4.
- [14] Abu K., Loogane M., Rana M., Naidoo N.,(2006). a quantitative analysis of ionising radiation exposure to the hands, thyroid and whole body of orthopaedic registrars At King Edward Viii Hospital During Fluoroscopic Internal Fixation of The Lower Limbs. J. Al-Aqsa Unv., 10 (S.E.).

Author Profile



Yousif Mohamed Yousif Abdallah received the B.S., M.Sc. and PhD degrees and M.Sc. in nuclear medicine and Radiotherapy Technology from College of Medical radiological Science, Sudan University of Science and Technology in 2005, 2009 and 2013, 2014, respectively. During 2006 up to date, he is staying in College of Medical radiological Science, Sudan University of Science and Technology. He is now assistant professor and Consultant Radiation Therapist.

Maryem Milad Hemair is working in Faculty of Medical Technology, Alzawya University, Alzawya, Libya

Amel S. Algaddal is working in Sebha Infertility Center, Sebha, Libya